



# Teknokroma Capillary Columns



## TRB-BIODIESEL / TKM-BIODIESEL

- Glycerin and Mono-,Di-,Triglycerides analysis tested under EN14105/ASTM D6584 methods
- Chemical inertness guaranteed for a good response for glycerin analysis
- Low column bleed at high temperatures
- Two columns, silica (High temperature polymide) and metal treated stainless steel

## TRB-BIODIESEL / TKM-BIODIESEL

Internal Diam.(mm)	Length (m)	Film Thickness (µm)	Temp limits (°C)	Part. N°. (P/N)
<b>0,32 (Fused Silica)</b>	10 + 2 m x 0.53 mm retention gap attached using SS connector	0.10	400	<b>TR-G780143</b>
<b>0,28 (Metal)</b>	10 + 2 m x 0.53 mm retention gap attached using SS connector	0.10	400	<b>TR-G780147M</b>

### Analysis of Glycerin and Glycerides (EN14105/ASTM D6584) Low Bleed at 370°C

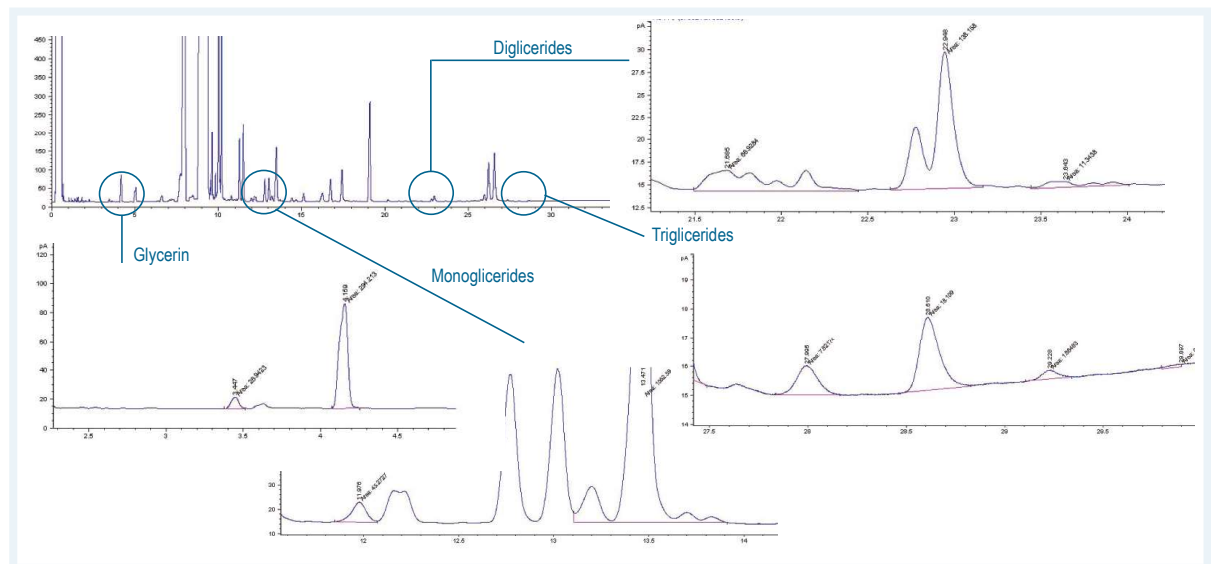

### Also for Biodiesel analysis

Methanol analysis (EN-14110)  
FAMES and Linolenic acid methyl ester analysis (EN-14103)

**TRB-1**, 30 m x 0.32 mm x 3.0 µm, P/N TR-113033  
**SupraWAX-280**, 30 m x 0.32 mm x 0.25 µm, P/N TR-830233