


NITRILES AND AMINES IN WATER

Column: **TRB-5A**, P/N TR-210532
Dimensions: 30m x 0.25mm x 0.5µm
Injection: 0.5µL (0.1mg/mL) acquos sample , split 1:25, 200°C
Carrier Gas: He, constant pressure 12 psi (82.7 KPa).
Oven Temperature: 50°C(5min) @ 15°C/min to 200°C
Detector: FID, 280°C

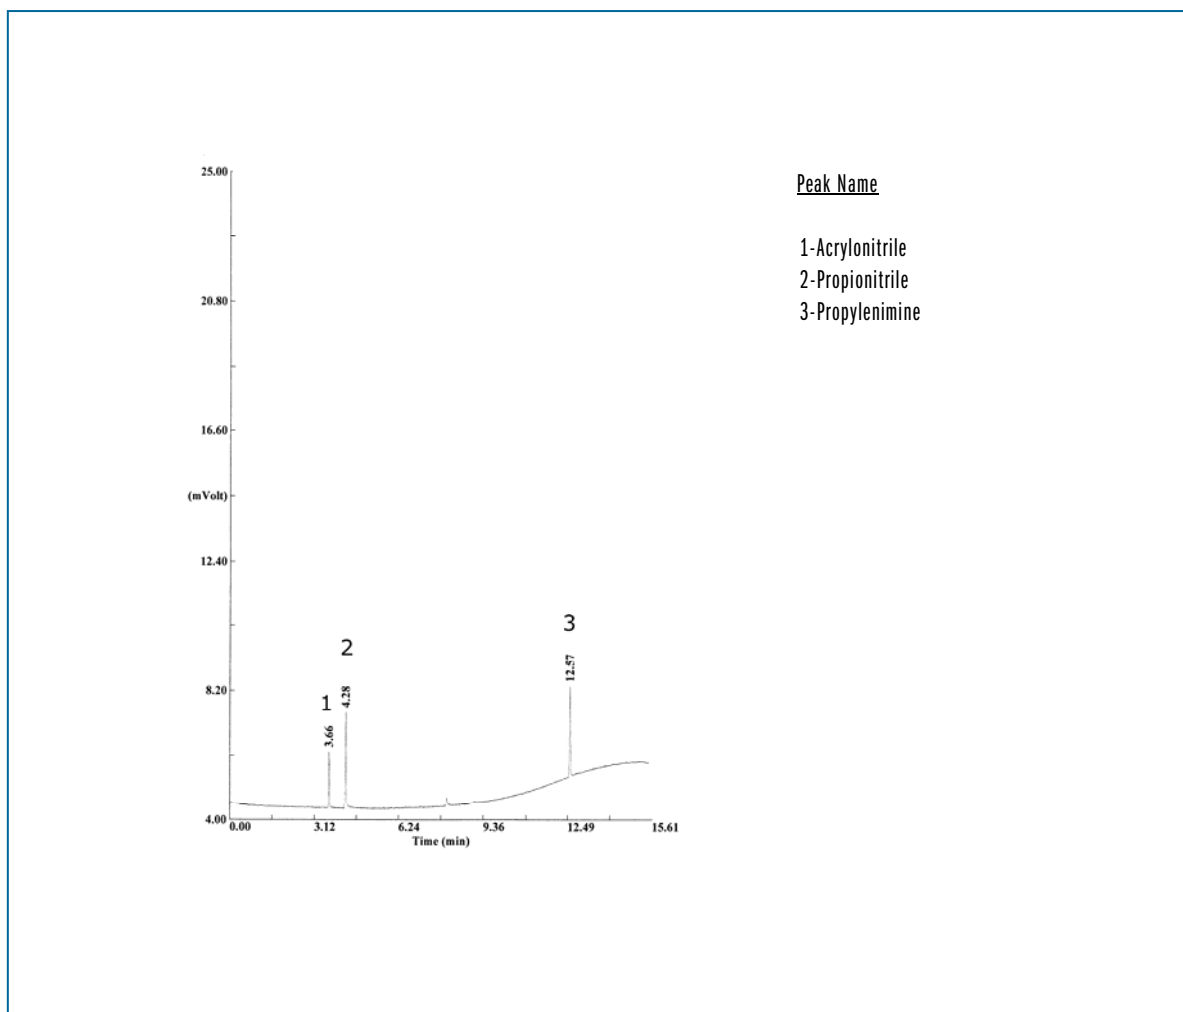

TKG 1020